

Welch Allyn® Spot™ Vision Screener Model VS100



Directions for use

Software version 3.1.XX

WelchAllyn®

Advancing Frontline Care™

© 2018 Welch Allyn. All rights are reserved. To support the intended use of the product described in this publication, the purchaser of the product is permitted to copy this publication, for internal distribution only, from the media provided by Welch Allyn. No other use, reproduction, or distribution of the publication, or any part of it, is permitted without written permission from Welch Allyn.

Welch Allyn assumes no responsibility for any injury to anyone, or for any illegal or improper use of the product, that may result from failure to use this product in accordance with the instructions, cautions, warnings, or statement of intended use published in this manual.

Welch Allyn® is a registered trademark of Welch Allyn.

Spot™ is a trademark of Welch Allyn.

Software in this product is Copyright 2018 Welch Allyn or its vendors. All rights are reserved. The software is protected by United States of America copyright laws and international treaty provisions applicable worldwide. Under such laws, the licensee is entitled to use the copy of the software incorporated with this instrument as intended in the operation of the product in which it is embedded. The software may not be copied, decompiled, reverse-engineered, disassembled, or otherwise reduced to human-perceivable form. This is not a sale of the software or any copy of the software; all right, title, and ownership of the software remain with Welch Allyn or its vendors.

This product may contain "free" or "open source" software (FOSS). To learn more about Welch Allyn's use and support of FOSS, please visit <http://www.welchallyn.com/opensource>.

For patent information, please visit www.welchallyn.com/patents.

For information about any Welch Allyn product, contact Welch Allyn Technical Support:
www.welchallyn.com/about/company/locations.htm.

DIR 80024271 Ver. A
Revision date: 2018-12

This manual applies to **REF** 901029 Vision Screener.



Welch Allyn, Inc.
4341 State Street Road
Skaneateles Falls, NY 13153 USA

- Introduction 1
 - Intended use 1
 - Indications for use 1
 - Contraindications 1
 - Symbols 2
 - Documentation symbols 2
 - Power symbols 2
 - Miscellaneous symbols 3
 - User Interface Symbols 3
 - Warnings, cautions and notes 5
 - Contents Checklist 7

- Controls, Display Window, and Connections 9
 - Features 9
 - Display Window 11
 - Subject Information Screen 12
 - Understanding the Results 13
 - Tools 14

- Setting up the Vision Screener 15
 - Charging 15
 - Powering the vision screener on and off 15
 - Tripod mount 15
 - Helpful hints 15
 - Wireless network configuration 16
 - To add/change the network name (SSID): 16
 - To add/change the WPA/2 PSK passphrase (password): 16
 - To add/change the WPA/2 EAP-PEAP username and password: 16
 - To add/change the WEP key (password): 16
 - To enable or disable the wireless capabilities on the vision screener: 17
 - To view advanced network settings: 17
 - Printer configuration 17
 - To select or change a default printer: 17
 - To configure a printer 17
 - To delete a printer 17
 - To reset the printer system 18
 - Adding a network printer 18
 - Adding a direct connect (USB) printer 18
 - Importing/exporting files 19
 - Export 19
 - Import 20
 - Custom banner 20
 - To add a custom banner 20
 - Web access 21
 - Licensing 21

- Vision Screener operation 23
 - Screening Environment 23
 - Screening a Subject 23

How to focus the vision screener	24
Monocular mode	25
Viewing the results	26
Understanding the Results.	27
Vision Screener criteria	28
Subjects	28
Troubleshooting	31
System restart	31
System freeze	31
Printer issues	31
Wireless issues	31
System messages	32
Cleaning the Vision Screener	35
Clean the Vision Screener	35
70 percent isopropyl alcohol	35
10 percent chlorine bleach solution	35
Specifications	37
Power supply specifications.	38
Vision Screener specifications	38
Screening capacity	38
Storing the equipment	39
Disposing of electronic equipment	39
EMC compliance	40
Emissions and immunity information.	41
FCC compliance statement	45
Vision Screener radio	46
International radio compliance	47
General radio compliance.	48
Industry Canada (IC) emissions	48
European Union	49
Vision Screener.	51

1

Introduction

This Directions for use manual is a comprehensive guide designed to help you understand the capabilities and operation of your Spot Vision Screener VS100. The information in this manual includes all options available with the Spot Vision Screener. The applicability of some sections of this manual depends on the configuration of your particular device. Read this manual thoroughly before attempting to use the device.

The vision screener is a hand-held instrument with a video display on the rear of the unit that provides subject visualization and alignment. Video display also provides user interface functionality for data input and display. The vision screener provides visual and audible cues to attract subject's attention and gaze. The device provides a fast data collect for easy evaluation of the most difficult pediatric subjects of limited compliance. Each screening provides simultaneous binocular assessment of the subject's refraction, pupil size and gaze.

Intended use

The Spot Vision Screener is intended to produce optical images that can help identify refractive errors and ocular misalignments by detecting special light reflexes from each eye during screening. The Spot Vision Screener evaluates these light reflexes from the retina to estimate refractive error. It also estimates pupil size, pupil distance and eye gaze deviation. It is intended for use on subjects six months of age through adults.

Indications for use

The Spot Vision Screener is indicated for use by healthcare professionals or under the direction of a healthcare professional to screen or evaluate individuals for potential refractive errors associated with poor vision. This type of photoretinoscopy device is intended to help the healthcare professional assess whether the subject should be referred to an eye care specialist for further evaluation or simply be monitored at future screenings. This screening is not intended to replace a full eye examination.

Contraindications

The Spot Vision Screener has no known contraindications.

Symbols

For information on the origin of these symbols, visit <http://www.welchallyn.com/symbolsglossary> for the Welch Allyn symbols glossary.

Documentation symbols



Consult operating instructions/directions for use (DFU). A copy of the DFU is available on this website. A printed copy of the DFU can be ordered from Welch Allyn for delivery within 7 calendar days.



WARNING The warning statements in this manual identify conditions or practices that could lead to loss of data, illness, injury, or death.



CAUTION The caution statements in this manual identify conditions or practices that could result in damage to the equipment or other property.

Power symbols



Rated power input, DC



Battery inside (Not user replaceable)



Power On/Off



USB port



DC power input port, Center pin positive

Miscellaneous symbols

Equipment is not protected against the ingress of liquid

IPXØ

Non-ionizing electromagnetic radiation



This symbol is applicable for EC member countries only. To avoid potential negative consequences for the environment and possibly human health, this instrument should be disposed of (i) for EU member countries - in accordance with WEEE (Directive on Waste Electrical and Electronic Equipment) or (ii) for all other countries, in accordance with local disposal and recycling laws.

User Interface Symbols

Battery status/level indicator



Battery charging



Wireless On/Off button



Connected to the wireless network



No wireless network in range



No IP address assigned by the router



Unknown network



Cannot connect to configured network



Sound off



Sound on



Continue



Back



Exit



Print job in progress



Warnings, cautions and notes



WARNING The warning statements in this manual identify conditions or practices that could lead to loss of data, illness, injury, or death.



CAUTION The caution statements in this manual identify conditions or practices that could result in damage to the equipment or other property.



WARNING Risk of electric shock. All signal input and output (SIP/SOP) connectors are intended for connection of only other medical devices, medical systems or non-medical devices complying with IEC 60601-1, or other IEC standards appropriate to the device. For example, a printer connected via USB must comply with IEC 60950. Connecting additional unapproved devices to the device might increase chassis or patient leakage currents.

WARNING Risk of electric shock. No modification of this equipment is allowed.

WARNING Risk of electric shock. Do not open the device or attempt repairs. The device has no user-serviceable internal parts. Only perform routine cleaning and maintenance procedures specifically described in this manual. Inspection and servicing of internal parts shall only be performed by qualified service personnel. Attempt to modify this device may result in bodily harm and will void product warranty.

WARNING Risk of electric shock. Do not allow the patient to make contact with accessible conductive parts (DC adaptor output connector, power input connector and USB port). Additionally, you should not make contact with the patient and any accessible conductive parts at the same time.

WARNING To avoid a possible explosion, do not use the device in the presence of flammable anesthetics: mixtures containing air, oxygen, or nitrous oxide.

WARNING Risk of data loss. If a reboot is required during a system freeze, data loss, such as printer configuration and subject data, can occur.

WARNING Lithium ion battery. Risk of fire, explosion, and burns. Do not handle or disassemble the battery pack.

WARNING Use only accessories approved by Welch Allyn. Visit www.welchallyn.com. The use of any other accessories can result in inaccurate patient data, can damage the equipment, and can void your product warranty.

WARNING Injury risk and equipment damage risk. When charging the device, properly secure all DC transformer cords to minimize trip hazards.

WARNING Patient injury risk. Verify patient identity on the device after manual entry and before printing or transferring patient records.

WARNING False positive and false negative results may occur in a healthcare screening. Vision screening does not replace a complete eye examination by an ophthalmologist or optometrist.

WARNING The use of screening results for recommending therapy is reserved exclusively for eye care professionals.

WARNING The screening results may not be used directly for the prescription of corrective eyewear.



Caution The device contains high-quality, fragile parts. Do not subject it to physical shock.

Caution Do not use the wrist strap as a means to carry the device; it is not designed to carry the weight of the device.

Caution The device is not waterproof. If you accidentally drop it into liquid or liquid is spilled on the device, contact Welch Allyn Technical Support immediately. If minor water droplets are found on the device, wipe off with a soft dry cloth.

Caution Do not store the device in the foam or case while the DC power adapter is plugged in; this may cause damage to the power cord and to the device.

Caution Do not leave the device in excessive heat or in direct sunlight. High temperatures can cause the device to malfunction.

Caution When plugging the DC power connector into the device, do not force the power connector into the device; this may cause damage to the device, which will not be covered under warranty.

Caution Do not push or scratch the touchscreen display with stiff or rigid objects. This may cause damage to the device. A stylus is acceptable for use with the device.

Note If the pupils are too small, the vision screener will notify you on screen to adjust the lighting in the room. For best results, subject's pupils should be 5mm or greater.

Note The power cord set may not be used with any other equipment other than the Welch Allyn Spot Vision Screener VS100.

Contents Checklist

The main shipping box contains the vision screener, Directions for use, and the Accessory box. The Accessory box contains:

AC Power Cord.

Power Supply/Charger.

Cleaning Cloth.

Velcro Cable Straps.

Note Please do not discard the box and foam. Damages incurred by shipping the device in non-approved packing material will void the limited warranty (see warranty for details).

If you purchased a carrying case, place the foam from the shipping box inside the carrying case for safer transport. Do not store your vision screener in the foam or case while the Power cord is plugged in.


2

Controls, Display Window, and Connections

Drawings and text are representative of the Spot Vision Screener with all available options.

Features


Rear View of Vision Screener

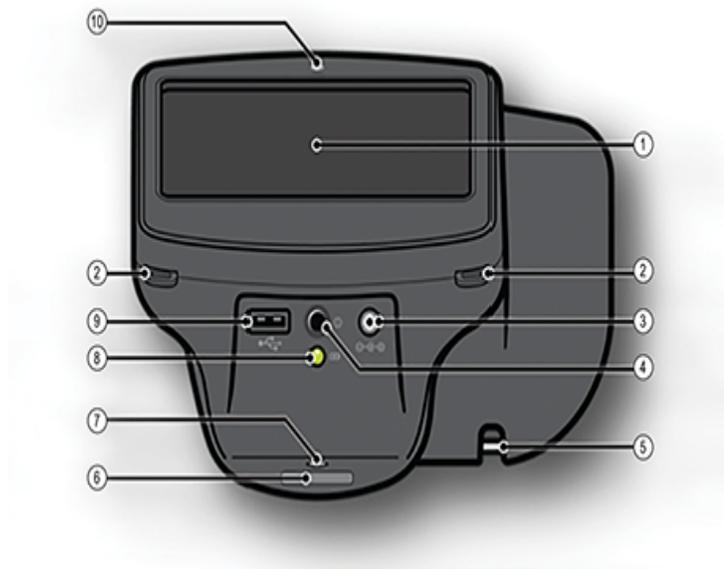

1	LCD Screen
2	Neck Strap Mount
3	AC Power Connector
4	Power Button
5	Wrist Strap Mount
6	Serial Number Label
7	Tripod Mount
8	Battery Charge Green LED Indicator (Flashing) or charged (Continuous)

9	USB Port
10	Ambient Light Sensor


Front View of Vision Screener

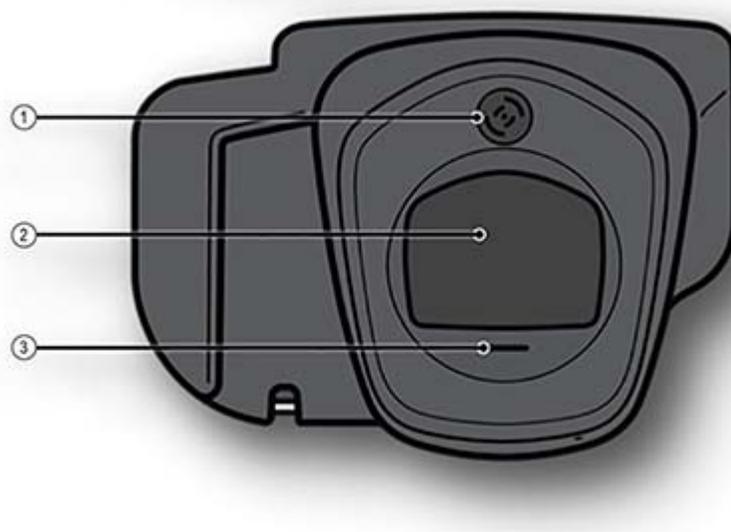

1	Range Finder
2	Front Glass
3	Speaker

Display Window

When the vision screener is powered on, the main menu or **Home** Screen will appear. If the vision screener is connected to a network, the network name and IP address will be visible in the upper left corner in the black bar.

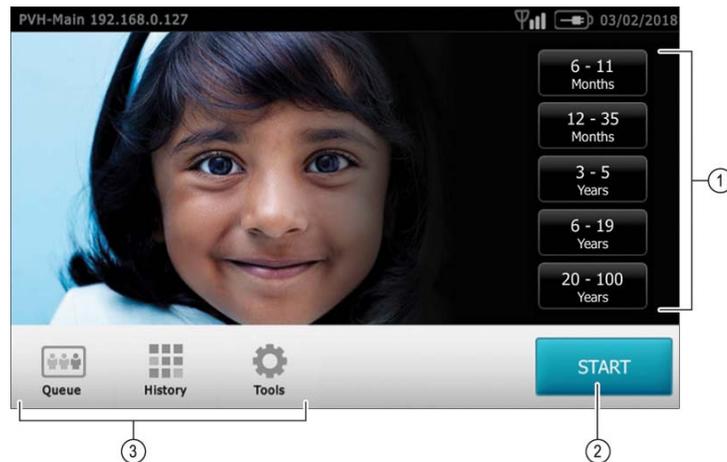

1. Age Range

To begin instant screening, with no personal subject data, select an age range of the subject from the **Home** screen. You will be able to enter subject data after the screening if desired.

2. START Button

The **START** button will allow you to:

- Enter subject information such as ID, First and Last Name, Gender and Date of Birth (DOB)/Age (Required)
- Find queued subjects (exact match on the ID screen)
- Begin the screening process (Binocular and Monocular available)
- Review and print screening results

3. Icons on Bottom of Screen

- **Queue** – View, select or search for queued subjects from a list to begin the screening process.
- **History** – View already screened subjects (completed records).
- **Tools** – A variety of options to customize the vision screener.

Subject Information Screen


On the subject information screen, confirm all data is correct. You can modify information by touching the field you wish to change. After the change is completed select **OK** and you will come back to the subject information screen. **Date of Birth/Age** is required and will highlight in red if there is no age or if it is not a valid birthdate or age (under 6 months). Select **GO** to begin the screening process.

The screenshot shows the 'Subject Information' screen on a mobile device. The title bar at the top reads 'Subject Information' and includes a date of '10/30/2015'. The main content area contains the following fields and options:

- SUBJECT ID:** 1792536
- NAME:** David Baker
- DATE OF BIRTH:** 40 years (marked as a required field with a red asterisk)
- EYEWEAR PRESCRIPTION:** None (selected), Glasses, Contacts
- GENDER:** Male (selected), Female

At the bottom of the screen, there is a 'Back' button on the left and a blue 'GO' button on the right.

Understanding the Results

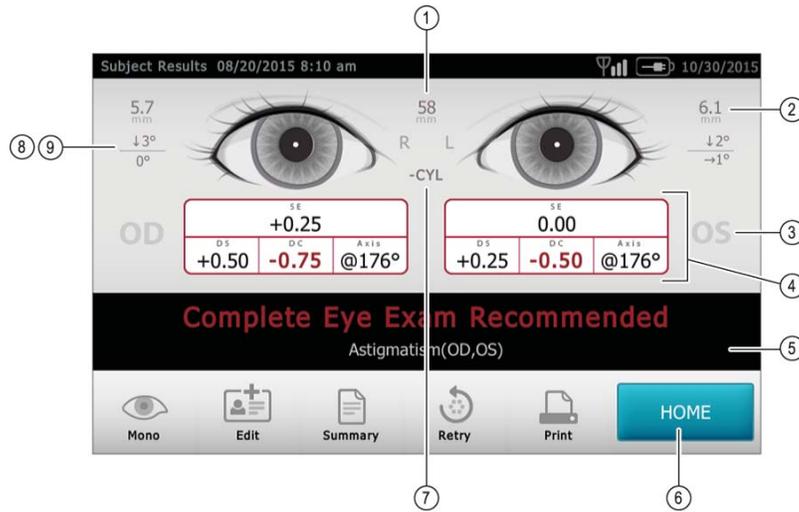

1	Pupillary Distance
2	Pupil Size Indicator
3	Right Eye (OD), Left Eye (OS)
4	Complete refraction SE - Spherical equivalent DS - Sphere DC - Cylinder Axis - Axis
5	Screening Result
6	Home
7	Cylinder Convention
8	Alignment Indicator
9	Degree, Horizontal, Vertical

Tools

The **Tools** menu will allow you to customize and configure the vision screener with the following options:

	Displays firmware version, software application version and serial number. Also displayed is a quick reference of important vision screener features, including memory storage levels of the device.
	View the age-based criteria settings used for exam recommendations that are currently active on the vision screener.
	Allows you to set the current date and time for your vision screener.
	Enables you to import and export using an inserted USB storage device.
	Location allows you to set a location for a screening and all subjects will be tied to that location.
	Allows you to connect the vision screener to a wireless network. You can manually enter your network name (SSID), select the security type, and enter the passphrase for your network. From this page you can view and change your TCP/IP settings.
	Allows you to configure a network printer and print a test page. It also lets you view printer status.
	Allows you to configure how data is displayed on the "Results" screen when a screening is complete. This includes data format, cylinder convention, displaying or hiding screening results and recommendations, setting default screening display and screening time-outs.
	Helps you set a security PIN for your device for added security. If enabled a PIN will be required whenever you start the device or upon waking it.
	Activates the license on the device.
	Allows you to select the language that will display on the vision screener.

3

Setting up the Vision Screener

Charging

1. Connect the provided DC cord set and power supply/charger together.
2. Gently lift the back of the vision screener to view the available connections.
3. Locate the DC power connector on the vision screener and connect the power supply/charger. The DC power connector on the power supply/charger will easily insert into the DC power connector on the vision screener. Using force to connect the power charger can damage the device and will void the warranty.
4. Plug the DC power cord into an available wall outlet to charge the device.

Powering the vision screener on and off

1. To turn the vision screener on, press and release the power button (start-up process takes approximately 30 seconds). Once powered on, you will see the Main Menu.
2. To turn the device off, press and hold power button for two seconds. A confirmation screen will appear to confirm shut down.
3. A flashing green light means the unit is charging, a steady green light means the unit is fully charged.

Tripod mount

The vision screener can be mounted to a standard photographic tripod. A ¼-20 threaded mount located on the bottom of the device is available for attaching a tripod.

Helpful hints

- **No activity on the vision screener** — After 60 seconds the screen will dim; after 5 minutes the screen will automatically turn black to conserve battery power. Tap the screen to 'wake up' the vision screener or press the power button. If the screen does not light up, plug in the power cord and try again.
- **Exporting/Clear All** — Verify you have successfully exported desired data to a USB drive before you select **Clear All**.
- **Routinely delete ALL records from the vision screener** — Go to the **History** screen and select **Clear All** icon. Select **Delete All Records**. You may also delete all queued records.
- **Avoid powering off during a screening** — Once the screening takes place, exit by selecting the **Exit** button, then power down the device normally.

- **Input Screen** — Holding down the **Back** button on any input (keyboard) screen will delete all data from the field.
- **Low Battery** — When the battery level reaches a very low level, a notice will appear to the user indicating they should insert the power cable or the device will shut down. If no power cable is inserted, the device will automatically shut down due to low voltage.

Wireless network configuration

From the **Tools** menu, touch  **Network**. Current network settings are displayed on the screen. To add or edit any of the fields, see instructions below. If they are correct, touch  (**Exit**) to be returned to the **Tools** menu.

To add/change the network name (SSID):

1. Touch the **SSID Name** field; a keyboard will appear.
2. Enter the SSID (case sensitive); select **OK** to save your changes and return to the previous screen. The **OK** button will turn dark when changes have been made and are available to be saved.

To add/change the WPA/2 PSK passphrase (password):

1. Set the encryption type to WPA/2 PSK and touch the **Passphrase** button; a keyboard will appear.
2. Enter the passphrase (case sensitive) and select **OK**.
3. On the Network screen, select **OK** to save changes, otherwise changes will not be applied.

To add/change the WPA/2 EAP-PEAP username and password:

1. Set the encryption type to WPA/2 EAP-PEAP and touch **Passphrase**; a keyboard will appear.
2. Enter the user name (case sensitive) and select **OK**.
3. Enter the network password (case sensitive) and select **OK**.
4. On the Network screen, select **OK** to save changes, otherwise changes will not be applied.

To add/change the WEP key (password):

1. Touch the **Passphrase** button; a keyboard will appear (this is only available when the security field is set to WEP or WPA).
2. Enter the WEP key (case sensitive password) and select **OK**.
3. On the Network screen, select **OK** to save changes, otherwise changes will not be applied.

To enable or disable the wireless capabilities on the vision screener:

1. Touch **Tools**.
2. Touch  **Network**.
3. Touch .
4. Touch **Enable/Disable**.

Note Wireless power can only be re-enabled after a device reboot. Touch **Enable** to automatically reboot.

To view advanced network settings:

1. Select **TCP/IP**. From here, you can also view your current TCP/IP address as assigned by your network.
2. For additional network configurations, select **Static** to manually configure your network address and settings. (Also available is the MAC address of your vision screener).

Printer configuration

The vision screener is capable of connecting and printing to most network capable Hewlett-Packard (HP) printers. The vision screener also contains some generic PCL drivers that can be used with non-HP printers, as well as a custom driver that supports the Brother QL-820NWB label printer.

Note In order to install the QL-820NWB on the vision screener, it must have QL-820 in its name on the network and you must select the driver labeled QL-820NWB from the driver list. Use Brother DK2205 Continuous Length Paper Tape or equivalent.

1. From the **Tools** menu, select the printer icon.
2. The next screen will list the available printers on the vision screener. This is a list of all printers already added to the vision screener.

To select or change a default printer:

From the printer list, find and select the desired printer (it will auto-highlight in blue.) If more than one printer is listed, touch **Set as Default** for the highlighted printer.

To configure a printer

Select a printer then press the **Edit** button to view printer status or print a test page.

To delete a printer

1. Select the printer from the available printer list; touch the **minus** button to delete.
2. A pop-up will appear asking you to confirm deletion of the printer.

To reset the printer system

This will delete all printers:

1. Touch the **Trash can** icon.
2. A pop-up will appear; touch **Delete**. This will remove all current printer configurations.

Adding a network printer

1. From the **Printers Available** screen, select the plus sign to add a printer.
2. If any printers are found on the network, they will appear in the list. If your printer is not shown, select **+ Add New Printer** at the top of the screen or you can select the printer you wish to add then press the continue icon.

Note Make sure you are connected to a wireless network with available printers for the vision screener to show printers available.

3. Review the printer details (Name, Driver and Location). To change or add settings touch the field you wish to change. If you need to add a driver, you can use the search feature by typing part of the driver name in the **Search** field.

Note PCL drivers are available for non-HP printers. It is not guaranteed that every printer will work with the vision screener.

4. Once changes have been made, select **Save**.
5. Once saved, the **Print Test Page** will appear dark.
6. A printer icon will appear in the menu bar indicating the job is processing. The number of jobs in the print queue will show up in the **Jobs** box at the top of the **Printer Details** screen, along with the current printer status.

Note If you are having a problem with your printer or a print job is stuck in the queue, select the reset button to clear the print job and reset the printer.

7. Return to the Printers Available screen and be sure to highlight the desired installed printer and set it as the default by selecting the **Set as Default** button.

Adding a direct connect (USB) printer

1. Connect the Vision Screener to a wireless network.
2. Connect the USB cable from the printer to the VS100's USB port.
3. Note the IP address of the VS100 from the main menu.
4. Visit the following URL on a computer on the same network:
`http://<ip_address_of_VS100>:631/`
5. Click on the Administration tab; under **Printers**, click on the **Find New Printer** button.
6. Click **Add This Printer** on the one listed with USB in the title, for example: HP ENVY 5530 series (HP ENVY 5530 series USB CN3C91S1N205XT HPLIP).

Note Give the printer a simpler name for ease of typing on the VS100, for example: use ENVY5530 instead of HP_ENVY_5530_series_USB_CN3C91S1N205XT_HPLIP.

7. Click **Continue**.
8. Choose **Make** and click **Continue**, for example: HP.
9. Choose **Model** and click **Add Printer**, for example: HP Envy 5530 Series hpjjs, 3.13.9 (en, en).
10. Click **Set Default Options**.
11. On the VS100, press **Tools**, then choose **Printer**.
12. Press the **+** arrow to add a new printer, then press the right arrow to choose **Add New Printer**.
13. Give the printer a name, for example: HP Envy 5530.
14. Press **Edit** under **Driver**, choose the proper driver for the printer.
15. Press **Edit** under **Location**, type in `ipp://127.0.0.1/printers/<printer_name>`, for example: `ipp://127.0.0.1/printers/ENVY5530`.
16. Press the **Save** button.
17. You may now press the **Print Test Page** button to confirm everything works.

Importing/exporting files

1. From the **Tools** menu, select **Import/Export** and you will be directed to the Import/Export screen.
2. Insert a USB storage device into the USB port on the vision screener (Recommended USB size is 8GB or larger).
3. Once the USB device is detected, the **Import** and **Export** buttons will be available for selection and you will see the USB symbol in the upper right black bar next to the wireless connectivity symbol.
4. The **Import** button will only become available if the vision screener recognizes a valid import file. Number of import files found will be shown on the screen.

Note If the buttons do not highlight within five seconds of inserting the USB drive, remove the USB, insert it into your PC and remove all files from the drive before attempting to retry.

Export

1. Select the **Export** button. If you wish to export one file containing no subject specific data select **Exclude Personal Data**. If you do not choose this option, then all data will be exported. Select **Export** button again to begin the export process.
2. Wait until the message "Export Finished successfully" displays, select **OK** then you may safely remove the USB drive from the vision screener.
3. The exported folder name on the USB will be "Spot_SerialNumber_YYYYMMDD_HHMMSS" (the folder labeled

“Spot_SerialNumber” will only contain screening data if inserted while screening subjects). It will contain:

- Spot Criteria file (located in the “import” folder).
- Spot Subjects Template file (located in the “db” folder).
- Spot Results file (located in the “db” folder).
- Spot Banner file (located in the “import” folder, will only be visible if custom banner was added).
- Subject PDF files (located in the “pdf” folder).

Note If the USB drive is removed prior to export completion, data transfer may be incomplete or become corrupted as a result.

Import

With the import function, you can import:

- Updated criteria files (SpotCriteria.csv)
- Future, queued, screening files (SpotSubjects.csv or Location.csv) By using a Location in the name of the file, this will default all subjects in the file to a location via the name of the file, ex LakeMary.csv would default to “LakeMary” as the location for all subjects in this file)
- Custom banner for the screening reports (banner.png) The file must follow the correct naming convention for a successful import (i.e., banner.png, SpotCriteria.csv, SpotSubjects.csv. Remember SpotSubjects can have a location as the name of the file).

Custom banner

Welch Allyn offers the ability to add a custom banner to the bottom of the printable reports. Please note that Welch Allyn does not supply custom banners. You will need to create your banner using the specifics below:

- Banner files must be named “banner.png”
- No larger than 1MB
- Image must be 1376 x 240 pixels

To add a custom banner

1. Place the banner.png file on the root/top-level directory of the USB.
2. Insert the USB in the vision screener. Go to “Tools”, then select **Import/Export**.
3. The import file option will highlight; select **Import**.
4. To verify that the file was imported successfully, screen a new subject or select a completed record and print the report. Your new banner will be printed on the bottom of the report.

Web access

When connected to a wireless network, the vision screener gives you the ability to view files from a web browser (Internet Explorer, Firefox, Safari, etc.) on a PC on the same network.

To access the webserver on the vision screener:

1. From your computer, open a web browser; enter the devices IP address in the address bar (this is located on the top black bar on the Home Screen).
2. You will be prompted to enter the username and password.

Username: *spot*
Password: *0000*

Note If you have enabled security on your device, the password will be your four-digit pin code.

3. Default will go to the Report folder. This contains the pdf folder where you can find subject PDF files.
4. To view the SpotResults.csv file change to the "db" directory.

Licensing

In order to use the screening functionality of the vision screener, the device needs to be licensed. If your device came new from the factory with this instruction document, your license is already installed and active. If you have updated the software on your device, the licensing will need to be updated as follows:

1. Connect an empty USB device to the vision screener USB port.
2. Go to "Tools", then touch **License**.
3. After a moment, a dialog box will appear indicating that the registration file has been exported to the USB drive.
4. Send the file titled spot-[serial number].reg to Welch Allyn Support at customerservice@welchallyn.com.

Welch Allyn Support will review your registration file and email you a valid license key. Once you receive the key, perform the following:

1. Save the file to the top level (root directory) of a USB Drive.
2. Insert the USB drive into the USB port on the vision screener.
3. From the **Tools** menu, select **License**. After a moment, a dialog box will appear indicating that the license file has been imported onto the device.

4

Vision Screener operation

Screening Environment

For optimal screening results, screen in an environment with lower level subdued lighting. Be sure to eliminate or block any sources of sunlight and/or incandescent light from reflecting on the subject's eyes. Florescent light is acceptable but note that the subject's pupil size can be affected and can decrease your chances of a successful screening.

Note If the pupils are too small, the vision screener will notify you on screen to adjust the lighting in the room. For best results, subject's pupils should be 5mm or greater.

Screening a Subject

1. Position yourself approximately 1 meter from the subject. If using a tripod, place the tripod approximately 1 meter from subject.
2. Start screening and slowly rotate the device upward to meet both of the subject's eyes. Adjust your distance from the subject until both eyes are clear on the screen. With a tripod, adjust the tripods position up or down and side to side until the subjects eyes are in focus on the screen.


A blue screen indicates you are too close or too far from the subject.

Note Keeping the vision screener even (on axis) with the subject's eyes will promote quicker results and help ensure you are not capturing other objects.

Position yourself with one foot in front of the other, slowly rock forward and back until the screen turns gray, indicating you are in the capture range. When using a tripod, move the tripod as needed to ensure focus on the subject's pupils until the screen turns gray.

3. Keep the vision screener device steady until the screening wheel appears, indicating the capture process is underway.
4. If you were unable to capture the subject's pupils with a successful screening, the screening cycle will be stopped. You can retry the screening, flag the record, try monocular mode, or return to the **Home** screen.
5. If the pupils are too small, the device will notify you on screen to adjust the lighting in the room to promote larger pupil size.

How to focus the vision screener

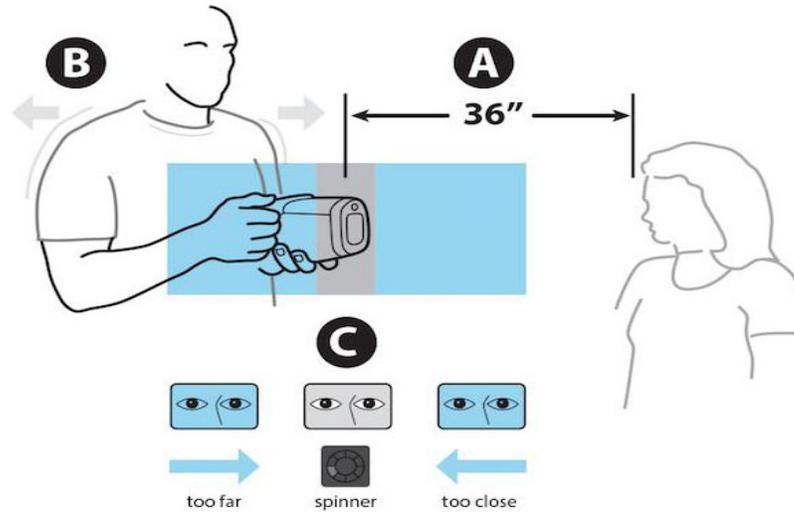

- A Position vision screener approximately 36 inches (1 meter) away from subject.
- B Hold vision screener close to body and lean forward and backward until the screen becomes gray.
- C Make small movements until the spinner appears on the gray screen.

Note Eyes should be wide open and kept on the center of the frame for best results.

Monocular mode

In monocular mode, you will be given the option to choose which eye to screen. This should be attempted when binocular screening does not capture the subjects' pupils.

After a binocular screening completes:

1. At the end of the binocular screening process, touch **Mono** and then select an eye to screen.
2. Touch the side of the screen that corresponds with the eye you would like to screen. (OD = subjects right eye; OS = subjects left eye).
3. When complete, you can repeat the process with the other eye by choosing **Mono** from the **Subject Results** Menu.

If a measurement times out:


1. If a measurement times out after an unsuccessful binocular screening, touch **Mono** and then select an eye to screen.
2. Touch the side of the screen that corresponds with the eye you would like to screen. (OD = subjects right eye; OS = subjects left eye).
3. When complete, you can repeat the process with the other eye by choosing **Mono** from the **Measurement Options** Menu.

Viewing the results


The results screen will appear at the end of the screening process.

All results viewing options are in the **Tools** menu under Results including: defaulting to a summary screen or the detailed results screen, hiding recommendations or screening results, cylinder convention options and raw or rounded data.

Measurements within range

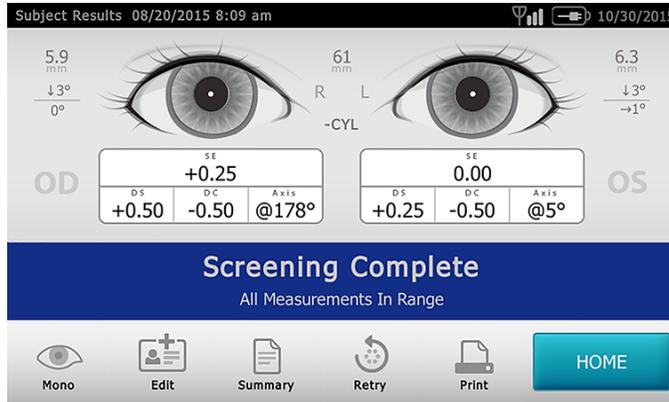


Eye exam recommended

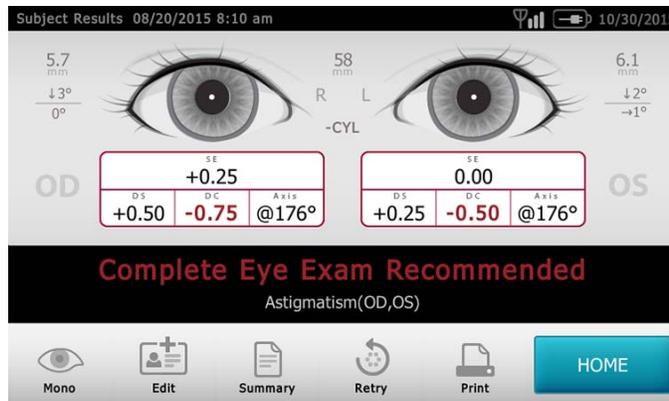

Understanding the Results

The figure below outlines the results screen and what it shows you:

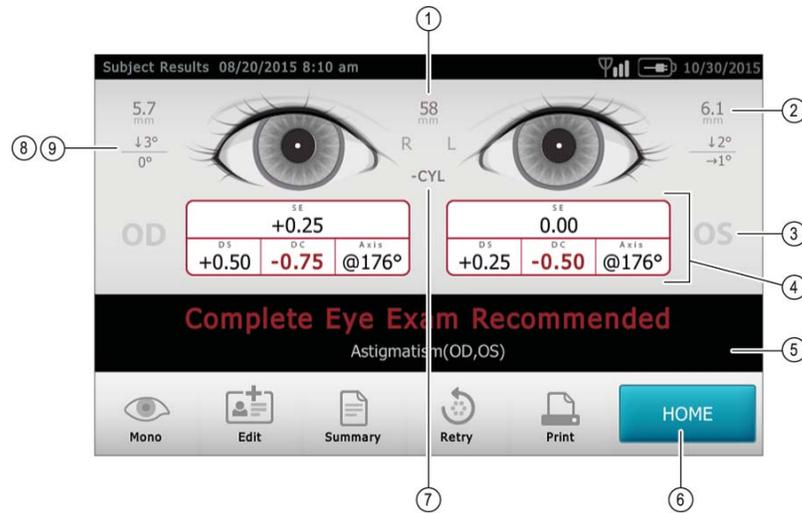

1	Pupillary Distance
2	Pupil Size Indicator
3	Right Eye (OD), Left Eye (OS)
4	Complete Refraction SE - Spherical equivalent DS - Sphere DC - Cylinder Axis - Axis
5	Screening Result
6	Home
7	Cylinder Convention
8	Alignment Indicator
9	Degree, Horizontal, Vertical

Results that are out-of-range are indicated in red.

Note Screening results provide an output that is either in- or out-of-range, accompanied by the appropriate statement in the device output display (“Screening Complete” or “Complete Eye Exam Recommended”). The displayed message is intended to prompt the caregiver to assess whether the subject should be referred to an eye care specialist for further evaluation or simply be monitored at future screenings.

Vision Screener criteria

Spot Vision Screener's criteria was developed in accord with the American Academy of Pediatric Ophthalmology and Strabismus (AAPOS) and American Academy of Pediatrics (AAP) recommendations for instrument based vision screening. The criteria is age specific to assist with early detection of amblyopic risk factors in children.

Note Any deviation from this criteria may lead to inaccurate readings.

To modify current screening criteria:

1. Perform an export and insert the USB drive into your PC.
2. Go to the USB drive folder and open the Spot folder that you just exported; select the import folder.
3. Copy the file "SpotCriteria.csv" to the top folder on the USB drive (the file cannot be within a folder). Once copied, open the file.
4. Make any desired changes using Microsoft Excel or compatible program.
5. Save file as a Comma Separated Value (.csv) file. You must make sure the file is called "SpotCriteria.csv". Eject the USB drive from your PC and insert into the vision screener.
6. Go to the **Tools** menu and select **Import/Export**. Select the **Import** button to import the updated criteria file.
7. To verify the file was imported successfully, go to the **Tools** menu and select **Criteria**; review new settings.

Note When custom criteria has been imported and is in use, there will also be a **Restore** button at the bottom of the screen. This button will prompt the user to confirm they want to revert to the default criteria that was shipped with the device. By confirming, the custom criteria will be deleted from the vision screener and replaced with the default criteria.

Subjects

The vision screener gives you the ability to populate a subject list for queued subjects.

1. Perform an export, once complete, remove the USB drive from the vision screener and insert it into your PC.
2. Select the Spot folder that was just created.
3. Select the "db" folder, then select the "SpotSubjects.csv" file.
4. The SpotSubjects.csv file contains six columns; do not change any of the column headings. Simply add information to the columns as shown below:

Note You may add a column before the Patient ID column and call it Location if you need to create specific locations for each subject.

- **Patient ID** — You can use any combination of alpha, numeric characters and symbols. This field is used for quick subject look-ups.
- **First Name** — Enter the first name. Use any combination of alpha characters.

- **Last Name** — Enter the last name. Use any combination of alpha characters.
- **Date of Birth** — Enter the date of birth in the format MM/DD/YYYY. You can enter the age of subject in years, months or a combination of both. This field is **required** for the import to work.

For example: If a subject were 2 years and 10 months old, you would enter 2Y10M. Use numeric and alpha characters.

- **Gender** — Select Male or enter M; select Female or enter F. Alpha characters only; leaving the field blank will default to no gender identified.
- **Eyewear prescription** — Select None, Glasses, or Contacts. By leaving the field blank, 'None' will be set as the default.

After updating the import file:

1. Confirm the file is saved as a Comma Separated Values (.csv) file.
2. Verify file name is 'SpotSubjects.csv' or 'DesiredLocation.csv'.

Note If labeling your subject file(s) with a location, the vision screener will import all files found on the USB drive at the same time.

3. Follow the import procedures to load the file onto the vision screener. To verify the file was imported successfully: Return to the **Home** screen and go to the **Queue** icon to view the new records.

5 Troubleshooting

System restart

1. To power cycle the vision screener - press and hold the **On/Off** button until a confirmation screen appears. Select **Confirm** to power off.
2. When the screen turns black, wait 30 seconds and then press the power button to turn the vision screener back on. Ensure the device has power by plugging in the power cord.

System freeze

In the event the vision screener locks up and is unresponsive to touch, you will need to perform a hard system reset.

1. Press the **On/Off** button.
2. If the **Power Off** window appears, select **Confirm** to shutdown the device.
3. If not, **press and hold** the **On/Off** button until the screen goes black, then release the **On/Off** button.
4. Wait about one minute then perform the normal start-up process.

Note This may cause some data loss (ex. printer configuration and subject data).

Printer issues

Check that your printer is turned on and has sufficient ink or toner:

1. Print a test print page directly from the printer.
2. After you confirm your printer is in proper working order, verify the printer is on a local network by printing to the printer from a PC on the same local network.
3. If all of the above are in working order perform a System Restart (see above).

Wireless issues

If you encounter problems connecting to a wireless network:

1. Check for the **Wireless** icon in the upper right corner. If the icon is red, try power cycling the vision screener first.
2. Verify all network settings are entered correctly.
3. If the settings are correct, try turning the vision screener off, then back on.

4. Check on the **Home** screen to see if your network name and IP address is identified in the upper left corner in the black bar.

Note Restarting helps to reinstate the connection to the network.

5. If the connection does not automatically reconnect, go to **Tools, Network**, select **Security Type**, reselect the correct type (None, WEP, WPA/2 PSK, and WPA/2 EAP-PEAP) then select the highlighted **OK**. This should re-instate the network connection.

System messages

Specific system messages may appear while operating the vision screener. If so, the information below will assist you in identifying what the messages indicate:

Message Text	Message Actions	Meaning	Action
Are you sure you want to delete the custom loaded criteria and restore system default criteria? To save your custom criteria, use the Export option in Import/Export tool.	Restore or Cancel	You have requested a restore to the factory default settings for the age based criteria settings. All setting will be lost if not saved.	Select Restore to continue or Cancel to continue using the device with the current criteria settings.
Unable to exclude personal data from recovered files, would you like to proceed?	Cancel or Continue	You have selected the option to exclude personal data from the current export operation that includes recovered data files. The device is unable to exclude personal data from recovered data files.	Select Cancel to abort the current export operation or select Continue to proceed with exporting the recovered data including personal information.
Export failed due to an internal error.	None	Data export failed.	Retry the export operation.
Would you like to delete the recovered files from this device?	Cancel or Delete	If an export contains recovered data files you will be asked whether the recovered files should be deleted or maintained on the device.	The device will continue to warn the user that there are recovery files to export until they have been deleted from the device following the export. Delete the recovery files once they have been exported to remove the message during system startup.
The database has been reset and recovery files have been built. (selecting export from the tools menu will transfer the recovery files).	OK	There was an internal error while restoring the patient history file. A backup recovery file has been generated and copied to the recovery area for export.	Touch Delete to delete the recovered files. Touch Cancel to retain the recovered files. If the recovered files remain on the device this dialog box will continue to be displayed once during each boot.
Battery is almost depleted, please plug into power source.	None	The battery is low and almost depleted.	Plug the device into the main power source to dismiss this dialog.
Unable to save PDF report for current subject	OK	There was an internal error that prevented the system from saving the PDF report for the current exam.	The file system may not have enough space, export data and clear the device history to free up additional storage space.
Sorry for the inconvenience. We need to reboot the device	OK or Cancel	Screening mode has encountered a problem and the device needs to be restarted.	Select OK to reboot the device or Cancel to continue using the device in Read Only mode. When operating in Read Only mode you will be able to review existing screening results. New screenings will not be possible until you have performed a reboot.
Problem encountered. The device needs to reboot.	Reboot	The system was not able to start and has attempted to correct the issue.	Reboot the device and try again. (To turn the device off, press and hold power button for two seconds.)

The screening system is not initialized.	None	The exam system did not initialize, or is unresponsive.	Reboot the device and try again. (To turn the device off, press and hold power button for two seconds.)
Un-calibrated device	None	The system has not been able to read the device configuration file.	Reboot the device and try again. (To turn the device off, press and hold power button for two seconds.)

For more information on troubleshooting or error messages, contact Welch Allyn's support team (refer to the inside cover of this manual for additional contact information).

6

Cleaning the Vision Screener

Clean the Vision Screener



WARNING Electric shock hazard. Before cleaning the vision screener, disconnect the DC power cord from the power outlet and the vision screener.



WARNING Liquids can damage electronics inside the vision screener. Prevent liquids from spilling on the vision screener.

If liquids are spilled on the vision screener:

1. Power down the vision screener.
2. Disconnect the power plug.
3. Dry off excess liquid from the vision screener.

If liquids possibly entered the vision screener, remove the vision screener from use until it has been properly dried, inspected, and tested by qualified service personnel.

Clean on a routine basis according to your facility's protocols and standards or local regulations.

The following agents are compatible with the vision screener:

- 70 percent isopropyl alcohol
- 10 percent chlorine bleach solution

Disinfect according to your facility's protocols and standards or local regulations.

70 percent isopropyl alcohol

Wipe the vision screener with a clean cloth slightly dampened with 70 percent isopropyl alcohol.

10 percent chlorine bleach solution

1. Wipe the vision screener with a clean cloth slightly dampened with a 10 percent bleach and water solution. Follow the cleaning agent manufacturer's guidelines.
2. Rinse with a clean cloth slightly dampened with water that meets EP and USP quality standards.
3. Allow the vision screener surface to dry for a minimum of 10 minutes before using the vision screener.

7

Specifications

The vision screener has the following characteristics:

- This vision screener DFU document is valid for software versions 3.1.xx.yy.
- The vision screener has been calibrated as part of the manufacturing process and does not require calibration henceforth.
- The external power supply/charger supplied is a Class II equipment and the vision screener is also a Class II equipment when connected to the external power supply/charger.
- The vision screener is internally powered by equipment (battery) when not connected to the external power supply/charger.
- Protection against electric shock, no applied part.
- The vision screener is rated IPX0 and thus not protected from the ingress of water.
- The vision screener is not suitable for use in the presence of a flammable anesthetic mixture with air or with oxygen or nitrous oxide.
- The vision screener is suitable for continuous operation.
- The vision screener quickly and easily detects vision issues across all age groups starting at 6 months.
- Welch Allyn suggests a battery replacement, at an appointed Welch Allyn repair facility, every 2.5 years at the owner's expense. The vision screener regular maintenance consists of wiping dust or dirt off the front glass surface and the LCD display as needed.
- The USB port shall only be used for software download/upload via a USB flash drive and shall not be cable connected to any other device.

Power supply specifications

Mfg: SL Power Electronics

Model: MENB1040A1503N01 or MENB1040A1541N01

Japanese Model: MENB1040A1503N02

Input Voltage: 90 – 264VAC (100 – 240VAC Nominal)

Input Frequency: 47 – 63 Hz

Input Current: 100VAC: 1.1A

Avg. Efficiency: 81-87% @ 0-50 W, ≥87% @ >51 to 250

Vision Screener specifications

Dimensions (cm/in): 21.6 cm x 17.1 cm x 12.1 cm (8 ½ in. x 6 ¾ in. x 4 ¾ in.)

Weight (lbs.): ~2.55

Wireless Network: 802.11 b/g/n

Operating Temperatures (°C): +10 to +40

Operating Humidity: 30% to 75% Relative Humidity (non-condensing)

Storage/Shipping Temperatures (°C): 0 to +50

Storage/Shipping Humidity: 0% to 95% Relative Humidity (non-condensing)

Storage/Shipping Atmospheric Pressure: 800 hPA to 1060 hPA

Expected Battery Life: 2.5 Years (Under Normal Usage)

Screening capacity

Note Screening results provide an output that is either in- or out-of-range, accompanied by the appropriate statement in the device output display (“Screening Complete” or “Complete Eye Exam Recommended”). The displayed message is intended to prompt the caregiver to assess whether the subject should be referred to an eye care specialist for further evaluation or simply be monitored at future screenings.

Refraction

Spherical equivalent:

- Range: -7.50D to +7.50D in 0.25D increments
- Accuracy: -3.50D to 3.50D, ± 0.50D
 - 7.50D to < -3.50D, ± 1.00D
 - > 3.50D to 7.50D, ± 1.00D

Cylindrical:

- Range: -3.00D to +3.00D in 0.25D increments
- Accuracy : -1.50D to 1.50D, ±0.50D
 - 3.00D to < -1.50D, ±1.00D
 - >1.50D to 3.00D, ±1.00D

Cylindrical axis:

- Range: 1 to 180 degrees in 1-degree increments
- Accuracy: ± 10 degrees (for cylinder values $> 0.5D$)

Pupil size:

- Range:
 - Years 0.5 - 19: 4.0 mm to 9.0 mm in 0.1 mm increments
 - Years 20 - 100: 3.0 mm to 9.0 mm in 0.1 mm increments
- Accuracy: ± 0.4 mm

Pupil distance:

- Range: 35 mm to 80 mm in 1 mm increments
- Accuracy: ± 1.5 mm

Screening principle: Eccentric photorefraction (photoretinoscopy) is used to estimate the magnitude of ametropia based on characteristics of the light reflex in the pupil.

Storing the equipment

When storing the vision screener, power cords, and accessories, observe the environmental storage conditions that are identified in the product specifications.

Disposing of electronic equipment

This product and its components must be disposed of according to local laws and regulations. Do not dispose of this product as unsorted municipal waste.

For more specific disposal or compliance information, see www.welchallyn.com/weee, or contact Welch Allyn Customer Service.

This device contains Lithium ion cells and other electronic materials. Please contact your local government authorities for proper electronic waste recycling or disposal methods at end of life.

Guidance and manufacturer's declaration

EMC compliance

Special precautions concerning electromagnetic compatibility (EMC) must be taken for all medical electrical equipment. This device complies with IEC EN 60601-1-2:2014.

- All medical electrical equipment must be installed and put into service in accordance with the EMC information provided in this *Directions for use*.
- Portable and mobile RF communications equipment can affect the behavior of medical electrical equipment.

This product complies with all applicable and required standards for electromagnetic interference.

- It does not normally affect nearby equipment and devices.
- It is not normally affected by nearby equipment and devices.
- It is not safe to operate this product in the presence of high-frequency surgical equipment.
- However, it is good practice to avoid using this product in extremely close proximity to other equipment.



WARNING Avoid using the vision screener adjacent to or stacked with other equipment or medical electrical systems because it could result in improper operation. If such use is necessary, observe the vision screener and other equipment to verify that they are operating normally.

WARNING Use only accessories recommended by Welch Allyn for use with the vision screener. Accessories not recommended by Welch Allyn might affect the EMC emissions or immunity.

WARNING Maintain minimum separation distance between the vision screener and portable RF communication equipment. Vision screener performance might degrade if you do not maintain a proper distance between equipment.

WARNING This device has not been tested for use in clinical environments near high-frequency surgical equipment and magnetic resonance imaging. Do not use this device in environments like these where electromagnetic disturbance is high.

Emissions and immunity information

Electromagnetic emissions

The device is intended for use in the electromagnetic environment specified below. The customer or user of the device should assure that it is used in such an environment.

Emission test	Compliance	Electromagnetic environment - guidance
RF emissions CISPR 11	Group 1	The device uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	The device is suitable for use in all establishments other than domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes, provided the following warning is heeded:
Harmonic emissions IEC 61000-3-2	Class A	 <p>WARNING This equipment/system is intended for use by healthcare professionals only. This equipment/ system may cause radio interference or may disrupt the operation of nearby equipment^a. It may be necessary to take mitigation measures, such as re-orienting or relocating the device or shielding the location.</p>
Voltage fluctuation/ flicker emission IEC 61000-3-3	Complies	

^a The device contains a 5-GHz orthogonal frequency-division multiplexing transmitter or a 2.4-GHz frequency hopping spread-spectrum transmitter for the purpose of wireless communication. The radio is operated according to the requirements of various agencies, including FCC 47 CFR 15.247 and RED Directive (2015/53/EU). The transmitter is excluded from the EMC requirements of 60601-1-2, but should be considered when addressing possible interference issues between this and other devices.

Electromagnetic emissions

The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Electrostatic Discharge (ESD) EN 61000-4-2	±8 kV contact ± 15 kV air	±8 kV contact ± 15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines ±1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	± 1 kV differential mode ± 2 kV common mode	± 1 kV differential mode ± 2 kV common mode	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<0 % U_T (>100 % dip in U_T) for 1 cycle 70 % U_T (30 % dip in U_T) for 25/30 cycles <0 % U_T (>100 % drop in U_T) for 0.5 cycles@ 0°, 45°, 90°, 135°, 180°, 225°, 270°, & 315° for 250/300 cycles	<0 % U_T (>100 % dip in U_T) for 1 cycle 70 % U_T (30 % dip in U_T) for 25/30 cycles <0 % U_T (>100 % drop in U_T) for 0.5 cycles@ 0°, 45°, 90°, 135°, 180°, 225°, 270°, & 315° for 250/300 cycles	Mains power quality should be that of a typical commercial or hospital environment. If the user of the device requires continued operation during power mains interruptions, it is recommended that the device be powered from an uninterruptible power supply or a battery.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

Note: U_T is the AC mains voltage prior to application of the test level.

Electromagnetic immunity

The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
			Portable and mobile RF communications equipment should be used no closer to any part of the device, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.
			Recommended separation distance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz	3 Vrms	$d = (1.17) \sqrt{P}$ 150 kHz to 80 MHz
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 1 GHz	3 V/m	$d = (1.17) \sqrt{P}$ 80 MHz to 800 MHz
Surge EN 61000-4-5	Differential mode: ± 1 kV Common mode: ± 2 kV	Differential mode: ± 1 kV Common mode: ± 2 kV	$d = (2.33) \times \sqrt{P}$ 800 MHz to 2,5 GHz where P is the maximum output power rating of the transmitter in watts (W) and d is the recommended separation distance in meters (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey ^a , should be less than the compliance level in each frequency range ^b . Interference may occur in the vicinity of equipment marked with the following symbol: 

Note1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

^aField strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast, and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the device is used exceeds the applicable RF compliance level above, the device should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the device.

^bOver the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

Recommended separation distances between portable and mobile RF communications equipment and the device

The device is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or user of the device can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the device as recommended below, according to the maximum output power of the communications equipment.

Separation distance at the transmitter Output maximum frequency (m)

Rated max. output power of transmitter (W)	150 kHz to 80 MHz $d = (1.17) \sqrt{P}$	80 MHz to 800 MHz $d = (1.17) \sqrt{P}$	800 MHz to 2,5 GHz $d = (2.33) \sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

Note 1: At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

Note 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

Test specifications for enclosure port immunity to RF wireless communications equipment

Test frequency (MHz)	Band ^a (MHz)	Service ^a	Modulation ^b	Maximum power (W)	Distance (m)	Immunity test level (V/m)
385	380 - 390	TETRA 400	Pulse modulation ^b 18 Hz	1.8	0.3	27
450	430 - 470	GMRS 460, FRS 460	FM ^c ±5 kHz deviation 1 kHz sine	2	0.3	28
710	704 - 787	LTE band 13, 17	Pulse modulation ^b 217 Hz	0.2	0.3	9
745						
780						
810	800 - 960	GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation ^b 18 Hz	2	0.3	28
870						
930						
1720	1700 - 1990	GSM 1800; CDMA 1900; GSM 1900; DECT; LTE Band 1, 3, 4, 25; UMTS	Pulse modulation ^b 217 Hz	2	0.3	28
1845						
1970						
2450	2400 - 2570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation ^b 217 Hz	2	0.3	28
5240	5100 - 5800	WLAN 802.11 a/n	Pulse modulation ^b 217 Hz	0.2	0.3	9
5500						
5785						

NOTE If necessary to achieve the IMMUNITY TEST LEVEL, the distance between the transmitting antenna and the monitor may be reduced to 1 m. The 1 m test distance is permitted by IEC 61000-4-3.

^a For some services, only the uplink frequencies are included.

^b The carrier shall be modulated using a 50 percent duty cycle square wave signal.

^c As an alternative to FM modulation, 50 percent pulse modulation at 18 Hz may be used because while it does not represent actual modulation, it would be worst case.

FCC compliance statement

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference and (2) this device must accept any interference received, including interference that may cause undesired operation.

Note This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in any environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.



WARNING Changes or modifications not expressly approved by Welch Allyn could void the user's authority to operate the equipment.

Vision Screener radio

The vision screener radio operates on 802.11 networks.

Wireless network interface	IEEE 802.11b/g/n
Frequency	2.400 GHz to 2.4835 GHz
Wireless data rates	WLAN11n(OFDM)7.2/14.4/15/21.7/28.9/30/43.3/45/57.8/60/65/72.2/90/120/135/150 Mbps WLAN11g (OFDM) 54/48/36/24//18/12/9/6 Mbps, WLAN11b (CCK) 11/5.5/2/1 Mbps
Output power	18.75 dBm EIRP
Modulation	OFDM, CCK
Channels	1 to 13
Security/encryption/authentication	WEP (64/128), AES, TKIP, WPA, and WPA2
Antenna	Pulse W1049B050 with I-PEX cable, Max Gain: 2.0dBi
Agency approvals	US: FCC 15.247:2014, KDB 558074 V3 Canada: (IC) RSS-210:2010 specification RSS-Gen:2010, RSS-102, IC:4168A-VS100 based on FCC testing Europe: 2014/53/EU Radio Equipment Directive

International radio compliance

Argentina	Ente Nacional de las Comunicaciones (ENACOM)	Contiene Modulo CNC I.D. C-15169
		
Brazil	Agência Nacional de Telecomunicações (ANATEL) 04569-15-08547	"Este equipamento opera em caráter secundário, isto é, não tem direito a proteção contra interferência prejudicial mesmo de estações do mesmo tipo, e não pode causar interferência a sistemas operando em caráter primário."
		
Mexico	Instituto Federal de Telecomunicaciones (Federal Telecommunications Institute—IFETEL)	This product contains an approved module, Model No. WATY, IFETEL No. RCPWEWA15-1278
Singapore	Infocomm Development Authority of Singapore (IDA) (新加坡通信管理局)	Singapore: Complies with IDS standard
South Africa		TA-2015/443

South Korea	Korea Communications Commission (대한민국 방송통신위원회 - KCC) Certification number: MISP-CRI-db3-WATY	This equipment is Industrial (Class A) electromagnetic wave suitability equipment and seller or user should take notice of it, and this equipment is to be used in the places except for home.
-------------	---	--



Class A Equipment
(Industrial Broadcasting & Communication Equipment) A 급 기기 (업무용 방송통신기자재)

이 기기는 업무용 (A 급) 전자파적합기기로서 판매자 또는 사용자는 이 점을 주의하시기 바라며, 가정외의 지역에서 사용하는 것을 목적으로 합니다.

Taiwan	National Communications Commission (國家通訊傳播委員會) NCC	低功率電波輻射性電機管理辦法 第十二條 經型式認證合格之低功率射頻電機，非經許可，公司、商號或使用者均不得擅自變更頻率、加大功率或變更原設計之特性及功能。 第十四條 低功率射頻電機之使用不得影響飛航安全及干擾合法
--------	--	--

Contains NCC I.D. CCAB16LP1620T8



This product can be used with the following restriction(s):

France — Outdoor use is limited to 10 mW EIRP within the band 2454 to 2483.5 MHz.

Norway — Does not apply for the geographical area within a radius of 20 km from the center of Ny-Ålesund.

Note Effective Isotropic Radiated Power (EIRP).

General radio compliance

The wireless features of this device must be used in strict accordance with the manufacturer's instructions as described in the user documentation that comes with the product. This device complies with Part 15 of the FCC rules, rules of the Canadian ICES-003 and the essential requirements of the 2014/53/EU Radio Equipment Directive as described below.

This device complies with EN62479, RSS-102 and 47 CFR 2.1093 for RF exposure.

Industry Canada (IC) emissions

This device complies with Industry Canada licence-exempt RSS standard(s). Operation is subject to the following two conditions: (1) this device may not cause interference, and (2) this device must accept any interference, including interference that may cause undesired operation of this device.

Le present appareil est conforme aux CNR d'Industrie Canada applicables aux appareils radio exempts de licence. L'exploitation est autorisée aux deux conditions suivantes : (1) l'appareil ne doit pas produire de brouillage, et (2) l'utilisateur de l'appareil doit accepter tout brouillage radioélectrique subi, même si le brouillage est susceptible d'en compromettre le fonctionnement.

This radio transmitter (IC ID: 4168A-VS100) has been approved by Industry Canada to operate with the antenna listed in the specification table.

This Class B digital apparatus complies with Canadian ICES-003.

Cet appareil numérique de la classe B est conforme à la norme NMB-003 du Canada.

European Union

This device complies with the essential requirements of the 2014/53/EU Radio Equipment Directive. The following test methods have been applied in order to prove presumption of conformity with the essential requirements of the 2014/53/EU Radio Equipment Directive:

This device is a 2.4 GHz wideband transmission system (transceiver), intended for use in all EU member states and EFTA countries, except in France and Italy where restrictive use applies.

In Italy the end-user should apply for a license at the national spectrum authorities in order to obtain authorization to use the device for setting up outdoor radio links and/or for supplying public access to telecommunications and/or network services.

This device may not be used for setting up outdoor radio links in France and in some areas the RF output power may be limited to 10 mW EIRP in the frequency range of 2454 – 2483.5 MHz. For detailed information the end-user should contact the national spectrum authority in France.

Czech	Welch Allyn tímto prohlašuje, že tento <i>RLAN device</i> je ve shodě se základními požadavky a dalšími příslušnými ustanoveními směrnice 2014/53/ES.
Danish	Undertegnede Welch Allyn erklærer herved, at følgende udstyr <i>RLAN device</i> overholder de væsentlige krav og øvrige relevante krav i direktiv 2014/53/EF.
Dutch	Bij deze verklaart Welch Allyn dat deze <i>RLAN device</i> voldoet aan de essentiële eisen en aan de overige relevante bepalingen van Richtlijn 2014/53/EC.
English	Hereby, Welch Allyn, declares that this <i>RLAN device</i> is in compliance with the essential requirements and other relevant provisions of Directive 2014/53/EC.
Estonian	Käesolevaga kinnitab Welch Allyn seadme <i>RLAN device</i> vastavust direktiivi 2014/53/EÜ põhinõuetele ja nimetatud direktiivist tulenevatele teistele asjakohastele sätetele.
Finnish	Welch Allyn vakuuttaa täten että <i>RLAN device</i> tyyppinen laite on direktiivin 2014/53/EY oleellisten vaatimusten ja sitä koskevien direktiivin muiden ehtojen mukainen.
French	Par la présente, Welch Allyn déclare que ce <i>RLAN device</i> est conforme aux exigences essentielles et aux autres dispositions de la directive 2014/53/CE qui lui sont applicables.
German	Hiermit erklärt Welch Allyn die Übereinstimmung des Gerätes <i>RLAN device</i> mit den grundlegenden Anforderungen und den anderen relevanten Festlegungen der Richtlinie 2014/53/EG. (Wien)
Greek	ΜΕ ΤΗΝ ΠΑΡΟΥΣΑ Welch Allyn ΔΗΛΩΝΕΙ ΟΤΙ <i>RLAN device</i> ΣΥΜΜΟΡΦΟΝΕΤΑΙ ΠΡΟΣ ΤΙΣ ΟΥΣΙΩΔΕΙΣ ΑΠΑΙΤΗΣΕΙΣ ΚΑΙ ΤΙΣ ΛΟΙΠΕΣ ΣΧΕΤΙΚΕΣ ΔΙΑΤΑΞΕΙΣ ΤΗΣ ΟΔΗΓΙΑΣ 2014/53/ΕΚ.
Hungarian	Alulírott, Welch Allyn nyilatkozom, hogy a <i>RLAN device</i> megfelel a vonatkozó alapvető követelményeknek és az 2014/53/EC irányelv egyéb előírásainak.

Italian	Con la presente Welch Allyn dichiara che questo RLAN device è conforme ai requisiti essenziali ed alle altre disposizioni pertinenti stabilite dalla direttiva 2014/53CE.
Latvian	Ar šo Welch Allyn deklarē, ka <i>RLAN device</i> atbilst Direktīvas 2014/53/EK būtiskajām prasībām un citiem ar to saistītajiem noteikumiem.
Lithuanian	Šiuo Welch Allyn deklaruoja, kad šis RLAN device atitinka esminius reikalavimus ir kitas 2014/53/EB Direktyvos nuostatas.
Malti	Hawnhekk, Welch Allyn, jiddikjara li dan RLAN device jikkonforma mal-htigijiet essenzjali u ma provvedimenti oħrajn relevanti li hemm fid-Direttiva 2014/53/EC.
Portuguese	Welch Allyn declara que este RLAN device está conforme com os requisitos essenciais e outras disposições da Directiva 2014/53CE.
Slovak	Welch Allyn týmto vyhlasuje, že RLAN device spĺňa základné požiadavky a všetky príslušné ustanovenia Smernice 2014/53ES.
Slovene	Šiuo Welch Allyn deklaruoja, kad šis RLAN device atitinka esminius reikalavimus ir kitas 2014/53/EB Direktyvos nuostatas.
Spanish	Por medio de la presente Welch Allyn declara que el RLAN device cumple con los requisitos esenciales y cualesquiera otras disposiciones aplicables o exigibles de la Directiva 2014/53/CE.
Swedish	Härmed intygar Welch Allyn att denna RLAN device står i överensstämmelse med de väsentliga egenskapskrav och övriga relevanta bestämmelser som framgår av direktiv 2014/53/EG.

Warranty

Vision Screener

Your Welch Allyn product, when new, is warranted to be free from original defects in material and workmanship and to perform in accordance with manufacturer's specifications under normal use and service. The warranty period* begins from the date of purchase from Welch Allyn, Inc. or its authorized distributors. Welch Allyn's obligation is limited to the repair or replacement of components determined by Welch Allyn to be defective within the warranty period. These warranties extend to the original purchaser and cannot be assigned or transferred to any third party. This warranty shall not apply to any damage or product failure determined by Welch Allyn to have been caused by misuse, accident (including shipping damage), neglect, improper maintenance, modification, or repair by someone other than Welch Allyn or one of its authorized service representatives.

* 1 (one) Year Limited Warranty

These express warranties are in lieu of any and all other warranties, express or implied, including the warranties of merchantability and fitness for a particular purpose, and no other person has been authorized to assume for Welch Allyn any other liability in connection with the sale of the Welch Allyn product. Welch Allyn shall not be liable for any loss or damages, whether direct, incidental or consequential, resulting from the breach of any express warranty, except as set forth herein.

WelchAllyn®

Advancing Frontline Care™

Material Number 729009